

FIG. 4



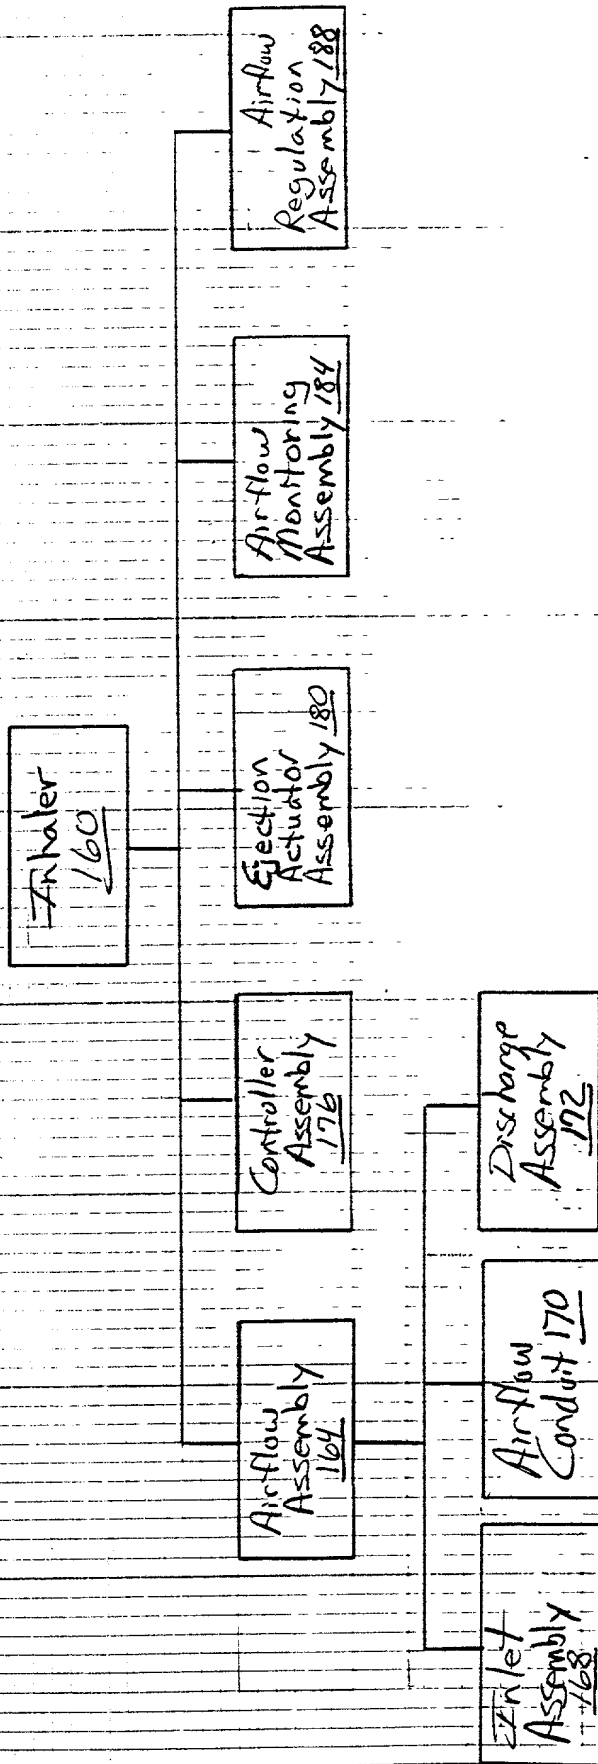


FIG. 6

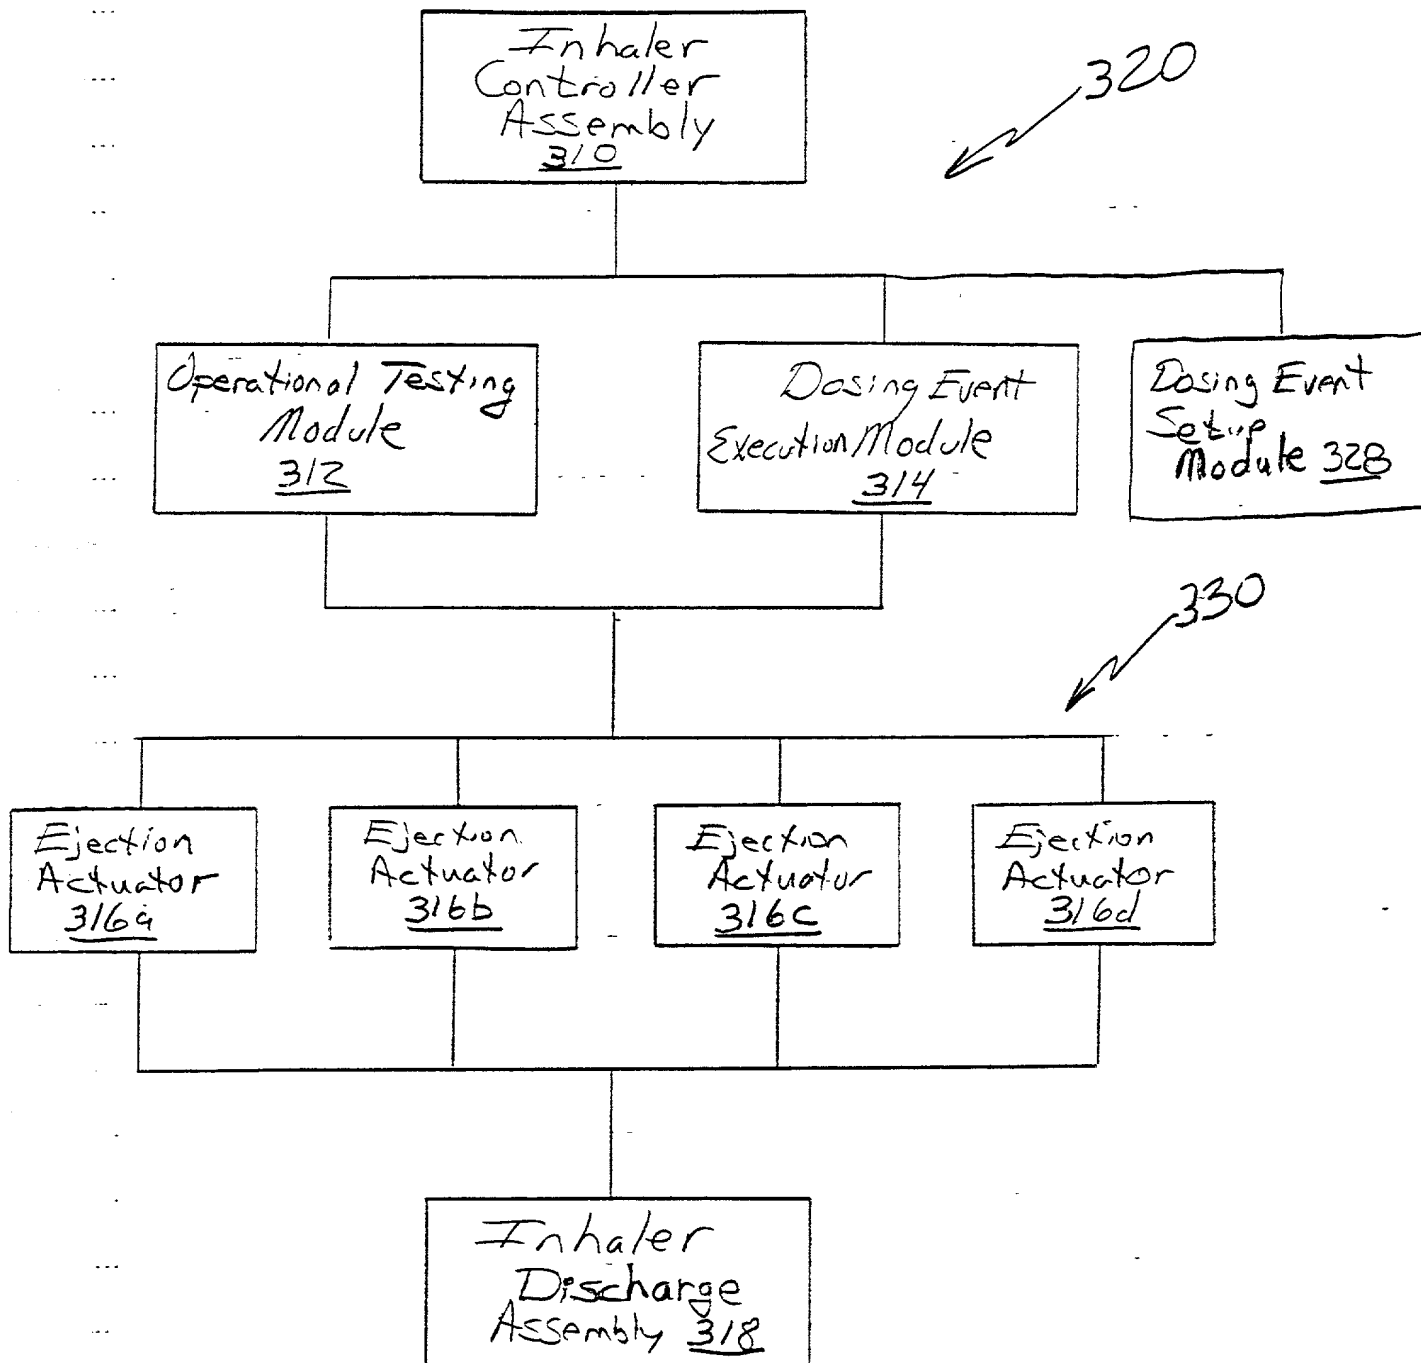


FIG. 7.

Inhaler  
Production  
Protocol 430



Specify Desired  
Number of Operational  
Ejection Actuators 316  
for Inhaler 320

422



Manufacture Inhaler  
320 With "Excess"  
Ejection Actuators  
316

424



Test Operation  
of Ejection  
Actuators 316

426



Designate Initial  
Ejection Actuators  
316 for Use by  
Inhaler 320

428

FIG. 8

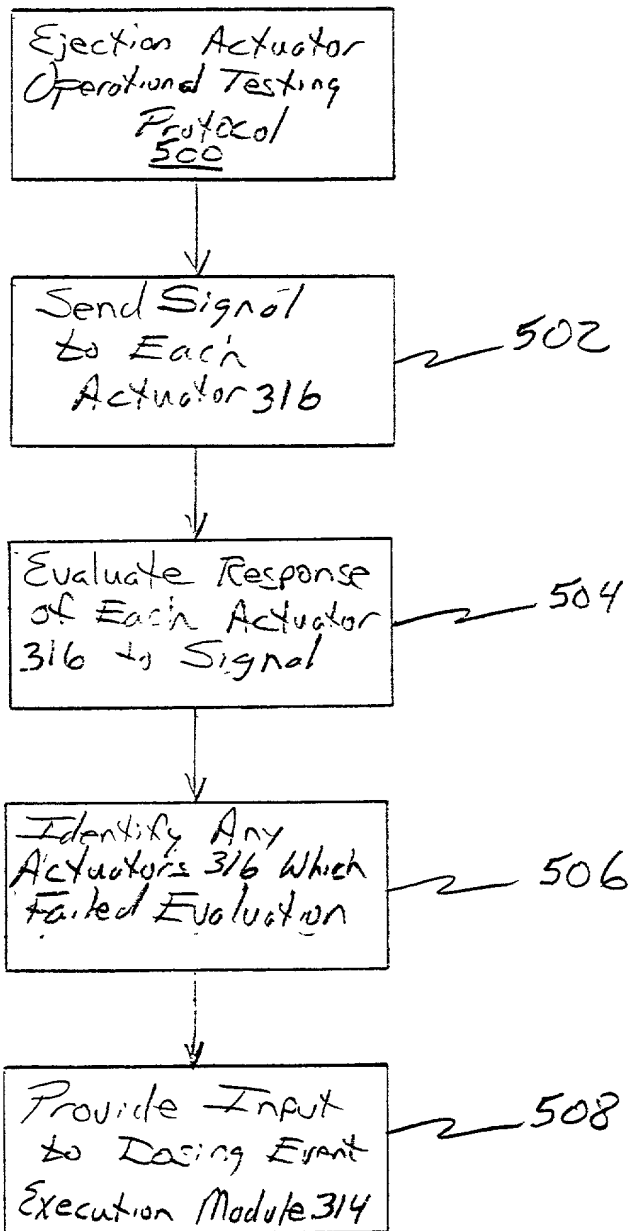
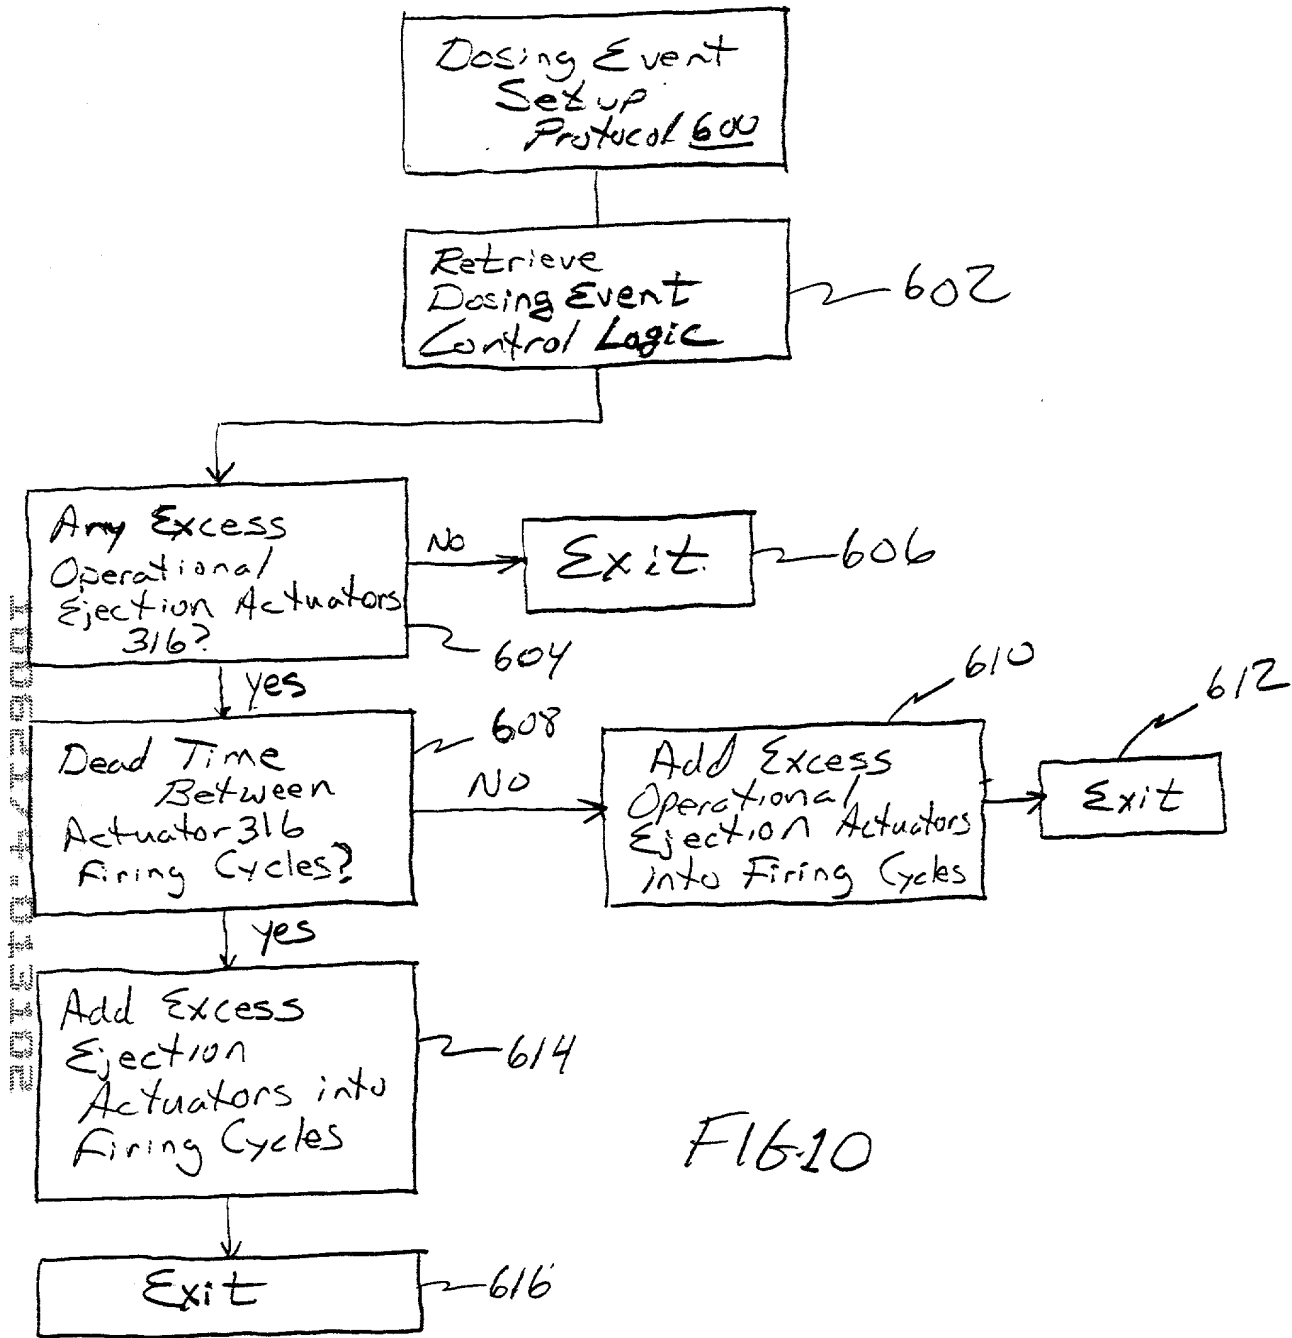


FIG. 9





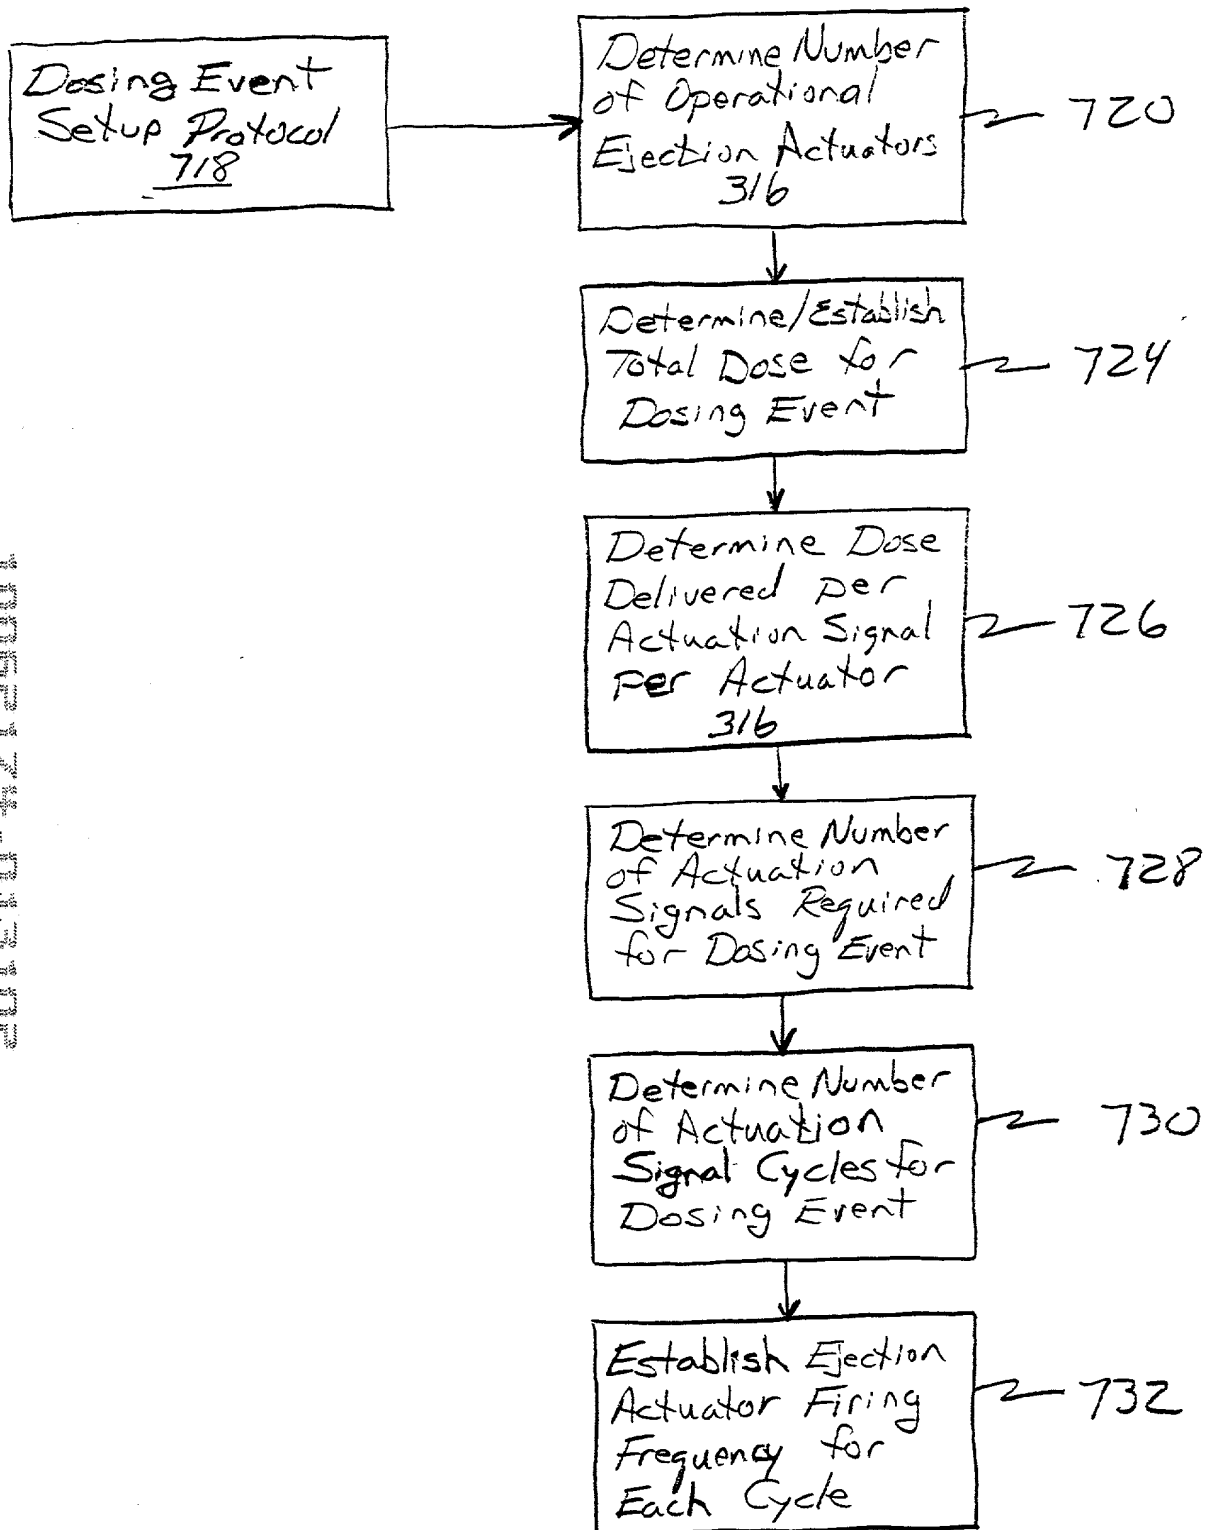


FIG. 11